



ExpressPlex™ 2.0 (96-well) Library Preparation Kit for Illumina® Sequencing Platforms

Catalog numbers:

- 301176:** ExpressPlex 2.0 (96-well) Library Preparation Kit, 4X96 Reactions - Set 1000
- 301177:** ExpressPlex 2.0 (96-well) Library Preparation Kit, 4X96 Reactions - Set 2000
- 301178:** ExpressPlex 2.0 (96-well) Library Preparation Kit, 4X96 Reactions - Set 3000
- 301179:** ExpressPlex 2.0 (96-well) Library Preparation Kit, 4X96 Reactions - Set 4000
- 301170:** ExpressPlex 2.0 (96-well) Library Preparation Kit, 1X96 Reactions - Any Index

User Guide

v20251110

Table of Contents

<u>Introduction</u>	<u>3</u>
<u>Molecular Diagram</u>	<u>5</u>
<u>Workflow Diagram</u>	<u>6</u>
<u>EP Green Workflow Diagram</u>	<u>7</u>
<u>ExpressPlex 2.0 Library Preparation Kit Components</u>	<u>8</u>
Considerations before you begin	
<u>User-Supplied Reagents, Equipment & Consumables, and Thermal Cycler Programs</u>	<u>11</u>
<u>Reagent handling</u>	<u>13</u>
Procedure	
<u>ExpressPlex 2.0 Reaction Setup (Manual, Full Plate)</u>	<u>14</u>
<u>ExpressPlex 2.0 Reaction Setup (Manual, Partial Plate)</u>	<u>15</u>
<u>ExpressPlex 2.0 Reaction Setup (Using Automated Liquid Handlers)</u>	<u>17</u>
<u>Thermal Cycling</u>	<u>18</u>
<u>Library Pooling</u>	<u>19</u>
<u>Library Pool Purification</u>	<u>20</u>
<u>Library Quantification and QC</u>	<u>22</u>
<u>Sequencing on Illumina Platforms</u>	<u>26</u>
 <u>Appendix A: Adjusting the Starting Sample Concentration</u>	 <u>27</u>
<u>Appendix B: Sample Sheet and Sequencer Guidelines</u>	<u>28</u>
<u>Appendix C: ExpressPlex Index Information and Demultiplexing Guidance</u>	<u>29</u>
<u>Appendix D: Library Quantification Options</u>	<u>31</u>
<u>Appendix E: Using PhiRx Indexed Control in Illumina sequencing</u>	<u>32</u>

Introduction

The patent-pending ExpressPlex 2.0 Library Prep Kit comes in both convenient 96-well and 384-well PCR plate configurations for high-throughput multiplexed library preparation. This upgraded version of ExpressPlex uses seqWell's high performance TnX™ transposase that was specifically engineered for NGS library preparation. Amplicons (>350 bp) and plasmid DNA are suitable standard inputs for the kits. ExpressPlex libraries are compatible with the Illumina MiSeq™, NextSeq™, iSeq™, and NovaSeq™ sequencing platforms.

Each ExpressPlex 2.0 (96-well) kit contains sufficient reagents to prepare Illumina-compatible libraries from 384 or 96 individual DNA samples. Libraries are typically prepared with 48 – 96 samples per pool, up to 384 samples per kit. For running fewer than 48 samples, please refer to additional criteria at the beginning of [section 1B](#). There are four different kits available for preparing libraries from 384 samples, providing a total of 1,536 barcode combinations that can be loaded on a single sequencing run. Set 1000 is recommended if running fewer than four 96-well plates (384 samples) per run with Illumina XLEAP-SBS chemistry. Guidelines for optimal batching can be found on our website. Please refer to Illumina's guidelines for optimal color balancing for different sequencing chemistries.



This multiplexed library preparation procedure is optimized for inputs of 1 - 40 ng of plasmid or amplicon DNA per 16 µl reaction, and typically generates library fragment lengths ranging from 400 – 1,200 bp. Library fragment length will depend on the quality and size of input DNA and magnetic bead cleanup ratio used. The primary advantages and benefits of using the ExpressPlex library preparation kits are a streamlined, one-step multiplexed library preparation workflow that automatically normalizes read output per sample across a 40-fold range of DNA input concentration, while minimizing labor and consumable costs. Using the ExpressPlex 2.0 (96-well) kit, a 96-plex library can be prepared for library QC and sequencing in under 120 minutes, with less than 30 minutes of hands-on time.

ExpressPlex 2.0 library preparation kits utilize a proprietary mixture of enzymes to tag input DNA with indexed adapters and amplify libraries all in a single reaction. Different full-length i7-indexed adapters tag the 96 DNA samples and barcoded libraries are amplified in separate wells, making for a highly efficient, one-step multiplexed library prep workflow. Each Indexing Reagent Plate contains a different i5 index that is applied to all samples within that plate ([Workflow Diagram](#) and [Appendix C](#)).


Each ExpressPlex 2.0 kit comes with a vial of PhiRx™ Indexed Control, which is a dual-indexed control library made from phiX174 genomic DNA and optimized for Illumina sequencing platforms,

particularly two-color systems like XLEAP SBS chemistry on NextSeq 1000/2000, MiSeq i100 and NovaSeq X. By improving color balancing for combinatorial indexed ExpressPlex 2.0 libraries (where there are only 1-4 i5 indexes used per kit), our PhiRx Indexed Control ensures cleaner, more accurate sequencing results and can be used as a 1:1 substitution for Illumina's PhiX Control V3. Please see [Appendix E](#) for PhiRx usage information.

ExpressPlex 2.0 Molecular Diagram

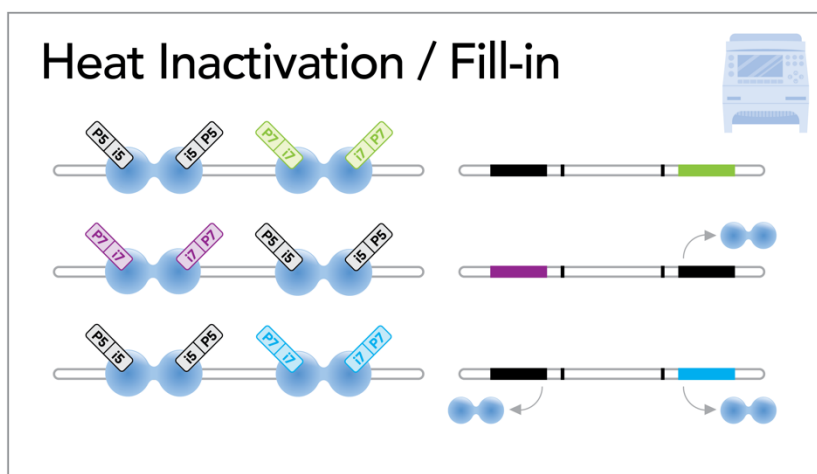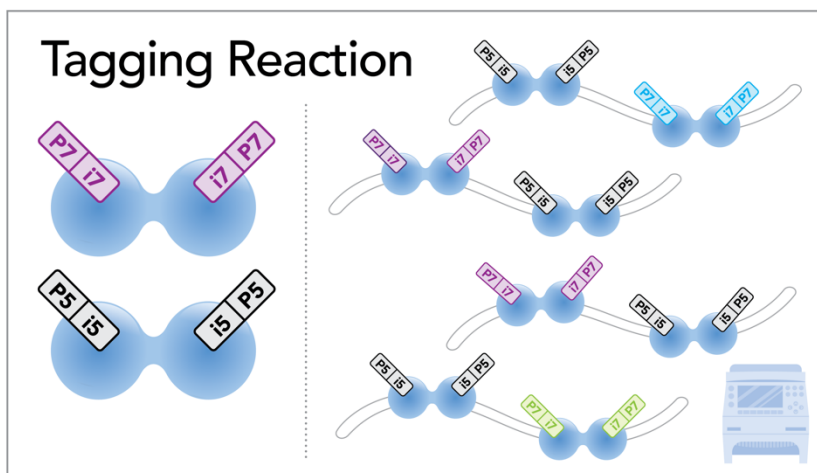


ExpressPlex 2.0 (96-well) Workflow Diagram

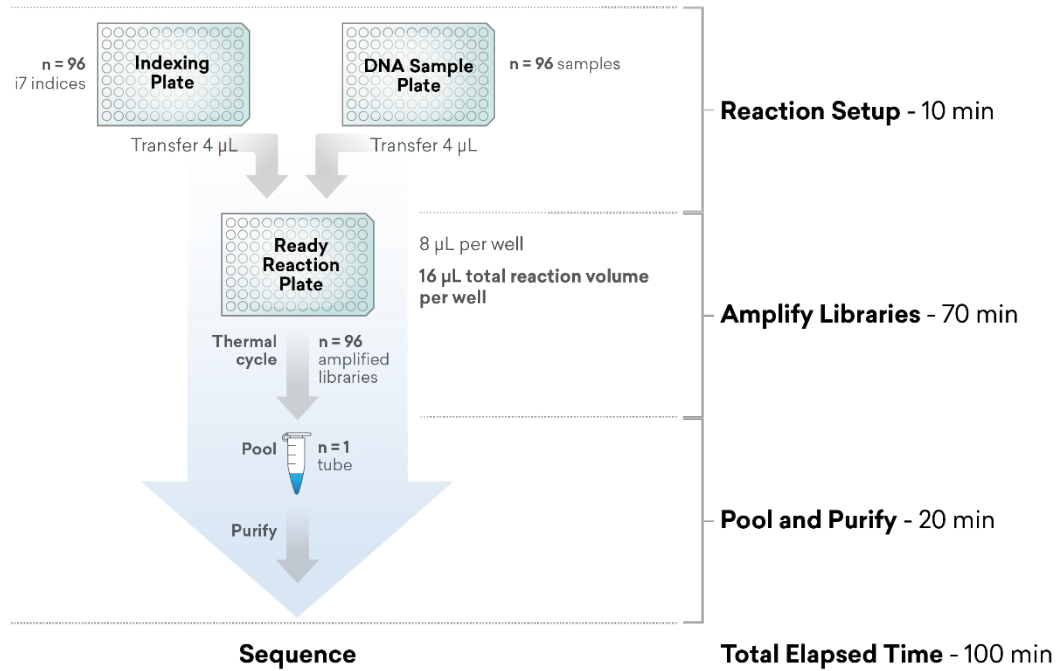

ExpressPlex 2.0 (96-well)

EP Green Automation Workflow Diagram

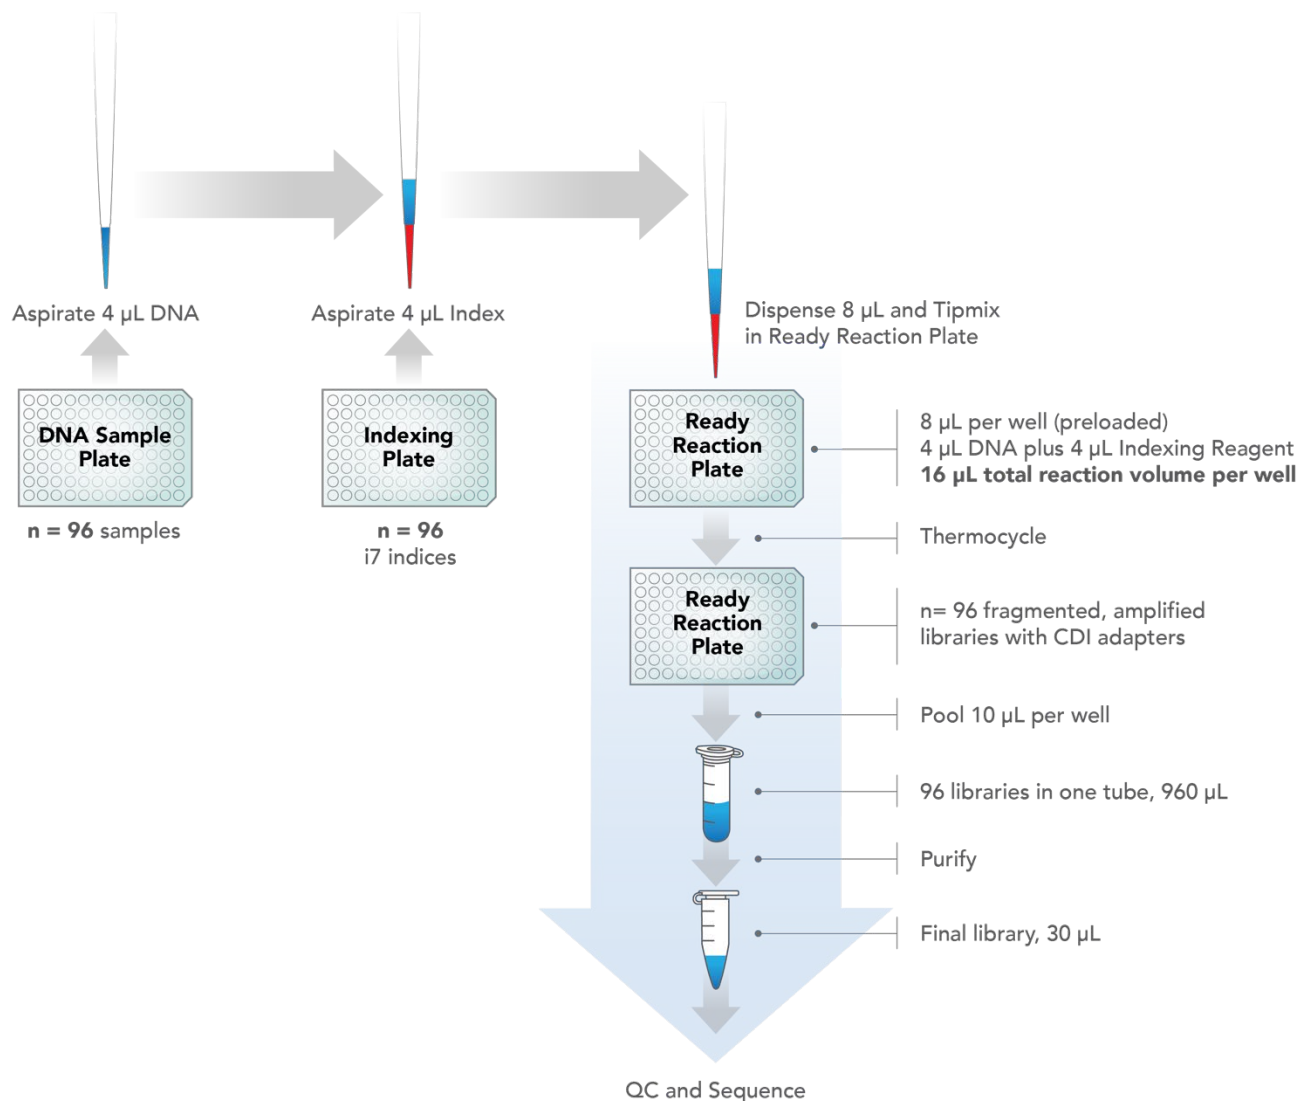

Kit Components

ExpressPlex 2.0 (96-well) Library Preparation Kit Components (4X96 Reactions)

ExpressPlex 2.0 (96-well) Library Preparation Kit, 4X96 - Set 1000

Catalog No.: 301176

Item	Component	REF	Description	Storage	Qty
1	Box 1 – 4X96 Indexing Reagent Plates - 1001, 1002, 1003, 1004	301171	Indexing Reagent Plates (96-well) in full-skirt, white PCR plates	-20°C	4
2	Box 2 – 4X96 Ready Reaction Plates	301175	Ready Reaction Plates (96-well) in full-skirt, red PCR plates	-20°C	4
3	MAGwise paramagnetic beads*	101003	5 ml of MAGwise beads in a 10 ml screwcap tube	4°C	1
4	PhiRx™ Indexed Control	301184	10 µL of 10nM PhiRx Indexed Control solution in a screwcap tube	-20°C	1

ExpressPlex 2.0 (96-well) Library Preparation Kit, 4X96 - Set 2000

Catalog No.: 301177

Item	Component	REF	Description	Storage	Qty
1	Box 1 – 4X96 Indexing Reagent Plates - 2001, 2002, 2003, 2004	301172	Indexing Reagent Plates (96-well) in full-skirt, white PCR plates	-20°C	4
2	Box 2 – 4X96 Ready Reaction Plates	301175	Ready Reaction Plates (96-well) in full-skirt, red PCR plates	-20°C	4
3	MAGwise paramagnetic beads*	101003	5 ml of MAGwise beads in a 10 ml screwcap tube	4°C	1
4	PhiRx™ Indexed Control	301184	10 µL of 10nM PhiRx Indexed Control solution in a screwcap tube	-20°C	1

* Larger volumes (15 ml) of MAGwise paramagnetic beads are also available to purchase separately (REF: 101002).

ExpressPlex 2.0 (96-well) Library Preparation Kit, 4X96 - Set 3000**Catalog No.: 301178**

Item	Component	REF	Description	Storage	Qty
1	Box 1 – 4X96 Indexing Reagent Plates - 3001, 3002, 3003, 3004	301173	Indexing Reagent Plates (96-well) in full-skirt, white PCR plates	-20°C	4
2	Box 2 – 4X96 Ready Reaction Plates	301175	Ready Reaction Plates (96-well) in full-skirt, red PCR plates	-20°C	4
3	MAGwise paramagnetic beads*	101003	5 ml of MAGwise beads in a 10 ml screwcap tube	4°C	1
4	PhiRx™ Indexed Control	301184	10 µL of 10nM PhiRx Indexed Control solution in a screwcap tube	-20°C	1

ExpressPlex 2.0 (96-well) Library Preparation Kit, 4X96 - Set 4000**Catalog No.: 301179**

Item	Component	REF	Description	Storage	Qty
1	Box 1 - 4X96 Indexing Reagent Plates - 4001, 4002, 4003, 4004	301174	Indexing Reagent Plates (96-well) in full-skirt, white PCR plates	-20°C	4
2	Box 2 – 4X96 Ready Reaction Plates	301175	Ready Reaction Plates (96-well) in full-skirt, red PCR plates	-20°C	4
3	MAGwise paramagnetic beads*	101003	5 ml of MAGwise beads in a 10 ml screwcap tube	4°C	1
4	PhiRx™ Indexed Control	301184	10 µL of 10nM PhiRx Indexed Control solution in a screwcap tube	-20°C	1

* Larger volumes (15 ml) of MAGwise paramagnetic beads are also available to purchase separately (REF: 101002)

ExpressPlex 2.0 (96-well) Library Preparation Kit Components (1X96 Reactions)**ExpressPlex 2.0 (96-well) Library Preparation Kit, 1X96 – Any Index****Catalog No.: 301170**

Item	Component	REF	Description	Storage	Qty
1	Indexing Reagent Plate (any index); Ready Reaction Plate	301169	Indexing Reagent Plate (96-well) in full-skirt, white PCR plate; Ready Reaction Plate (96-well) in full-skirt, red PCR plate	-20°C	1
2	MAGwise paramagnetic beads*	101003	5 ml of MAGwise beads in a 10 ml screwcap tube	4°C	1
4	PhiRx™ Indexed Control	301184	10 µL of 10nM PhiRx Indexed Control solution in a screwcap tube	-20°C	1

* Larger volumes (15 ml) of MAGwise paramagnetic beads are also available to purchase separately (REF: 101002).

User-Supplied Reagents, Equipment, Consumables, and Thermal Cycler Program

Reagents

- 100% Ethanol (molecular biology grade)
- Tris-HCl, pH 8.0
- Ultrapure Water (PCR grade)
- Quant-iT™ PicoGreen™ dsDNA Assay Kits (ThermoFisher P/N: P7589), or other validated dsDNA quantification assay
- Electrophoretic analysis reagents - Agilent TapeStation (High Sensitivity D5000 kit), Bioanalyzer (High Sensitivity DNA or DNA7500 kits), or Fragment Analyzer (High Sensitivity NGS Fragment Analysis Kit, DNF-474)

Equipment & Consumables

- Single-channel pipettors (1-20 µl, 20-200 µl, 100-1,000 µl)
- Multichannel pipettors (1-10 µl, 10-200 µl)
- Pipette tips (low-retention barrier tips)
- Eppendorf Tubes® (1.5 ml and 2 ml, DNA LoBind Tubes)
- PCR plate seals (must be evaporation-resistant)
- 96-well thermal cycler (compatible with fully skirted Bio-Rad Hard-Shell® 96-Well PCR plates and 8-tube PCR strips)
- Magnetic stand for 1.5 ml tubes
- 0.2 ml 8-tube PCR strips and caps/seals
- Benchtop centrifuge to pulse-spin tubes and 8-tube PCR strips
- Plate centrifuge
- Vortex mixer
- Electrophoretic analysis equipment - Agilent TapeStation, Bioanalyzer, or Fragment Analyzer
- Fluorometer for dsDNA quantification assay

Thermal Cycler Program EP2 TAG AMP (with lid-heating on at 105°C):

15	min	55°C	Tagging Reaction
5	min	75°C	Heat Inactivation / Fill-in
3	min	68°C	
5	min	79°C	
3	min	68°C	
5	min	83°C	
1	min	98°C	Initial denaturation
15	sec	98°C	Library Amplification (PCR) Use 12 cycles for plasmids Use 15 cycles for amplicons
30	sec	64°C	
1	min	72°C	
5	min	72°C	Final extension
Hold		4°C	

Before starting the procedure:

Review FAQs. FAQs can be found here: <https://seqwell.com/resource-category/faqs/>. Review these prior to your first run.

Measure and adjust input DNA concentration It is recommended that the user assay the DNA concentration of each plate of samples to be processed by PicoGreen or other validated dsDNA assay. This can be accomplished by measuring the concentration of a representative selection of samples. Globally adjust the average concentration of input DNA across each plate to 1.25 ng/μl (5 ng calculated input into final reaction) in 10 mM Tris-HCl, pH 8.0. Do not use EDTA-containing solutions (e.g., TE buffer) to dissolve or dilute input DNA because EDTA can suppress enzymatic activity. Refer to [Appendix A](#) for more detailed information on globally adjusting the average input DNA concentration. Refer to [section 1B](#) if working with <48 samples.

Program thermal cycler. For convenience, set up the thermal cycler program described in the previous page before starting.

Pulse-spin kit components. Liquids can condense or shift locations inside containers during shipment or storage. Before using the reagent plates and tubes, pulse-spin in a suitable centrifuge to gather the reagents at the bottom of the well or tube. If the kit components freeze during shipment or storage, thaw, mix and pulse-spin before use.

Equilibrate MAGwise Paramagnetic Beads to room temperature. MAGwise beads can be stored for up to 2 weeks at room temperature or for longer periods at 2 - 8°C. If stored cold, warm at room temperature for 30 minutes before use. Vortex to thoroughly resuspend beads prior to use. To transfer volumes accurately, pipette slowly and do not pre-wet pipette tips.

Prepare 80% ethanol fresh daily. You will need ~5 ml per sample plate.

Prepare 10 mM Tris-HCl, pH 8.0. Prepare 10 mM Tris-HCl, pH 8.0 from a concentrated stock solution diluted with ultrapure water (both molecular biology grade). Do not use EDTA-containing solutions (e.g., TE).

Safe stopping points are indicated in the protocol. For optimal results, proceed directly to the next step unless a safe stopping point is indicated.

Procedure

Key Items Before Starting:

- Refer to [Appendix A](#) for instructions to dilute input samples.
- ExpressPlex 2.0 reactions can be set up at room temperature.
- If processing more than one plate, multiple reaction plates may be set up and thermal cycled at the same time before proceeding to subsequent steps. (Immediate continuation after cycling is recommended).
- If manually preparing 96 samples at a time (full plate), proceed to [Section 1A](#) below.
- If manually preparing fewer than 96 samples at a time, proceed to [Section 1B on page 15](#).
- If using automation for reaction set up, proceed to [Section 1C on page 17](#).

1A. ExpressPlex Reaction Setup (Manual, full plate)

If preparing libraries from 96 samples at a time (full plate), complete the setup and thermal cycle directly in the Ready Reaction Plate as follows (see [Section 1B](#) on next page for alternate instructions on preparing <96 samples in a batch):

- Pre-label each **Ready Reaction Plate** with the index set ID and any other relevant information to allow easy identification of your samples.
- Pulse-spin one **Indexing Reagent Plate** and one **Ready Reaction Plate** in a tabletop centrifuge; then remove the heat seals carefully.

Do not try to puncture seals with pipette tips; seals must be removed by peeling.

- Carefully transfer 4 μ l of **Indexing Reagent** to each corresponding well of the **Ready Reaction Plate** with a multichannel pipettor, using new tips for each transfer.
- Next, transfer 4 μ l of input DNA (at approximately 1.25 ng/ μ l) to each well (one sample per well) of the **Ready Reaction Plate**. Mix thoroughly by pipetting up and down ten times at 4 μ l, being careful not to introduce excessive bubbles. Use clean tips for addition of each DNA sample.

Optional: If excessive bubbles are present after reaction setup, use a tabletop centrifuge to collapse the bubbles prior to proceeding.

- Seal the **Ready Reaction Plate**, and proceed directly to [Section 2: Thermal Cycling on Page 18](#).

1B. ExpressPlex 2.0 Reaction Setup (Manual, partial plate)

If preparing fewer than 96 samples (batches of 16 - 88 samples), complete the set up in a separate PCR-plate or strip tube(s) as follows.

For batches of fewer than 48 samples, ensure that these criteria are met:

- To ensure that enough yield is generated for sequencing, the minimum number of samples to be processed is 16.

NOTE: Batches of 8 samples may be processed ONLY IF an experienced user is comfortable with a final elution volume of 15 μ l.

- Measure and adjust input DNA concentration. Assay the DNA concentration of each sample to be processed by PicoGreen or other validated dsDNA assay. Adjust the concentration of input DNA to a minimum concentration of 2.5 ng/ μ l and a maximum of 10 ng/ μ l in 10 mM Tris-HCl, pH 8.0. Depending on pooling size, it is recommended to use higher inputs of DNA. Do not use EDTA-containing solutions (e.g., TE buffer) to dissolve or dilute input DNA because EDTA can suppress enzymatic activity. For WGS we recommend using high quality DNA input (DIN >7) for optimal results. Reach out to support@seqwell.com if processing samples with lower quality DNA.
- a. Pulse-spin one **Indexing Reagent Plate** and one **Ready Reaction Plate** in a tabletop centrifuge.
 - b. Only cut and peel the heat seal from the wells of both the **Indexing Reagent Plate** and **Ready Reaction Plate** corresponding to the total number of samples that will be processed. This may be done by *carefully* using a razor blade to cut the seal.

The **Indexing Reagent Plate** and **Ready Reaction Plate** can be thawed and refrozen up to 12 times without impacting performance.

- c. Carefully transfer 4 μ l of **Indexing Reagent** from the unsealed wells to each corresponding unsealed well of **Ready Reaction Plate** with a multichannel pipette. Use new tips for each column transfer.
- d. Next, transfer 4 μ l of input DNA (at approximately 2.5 - 25 ng/ μ l) to each well (one sample per well) of the **Ready Reaction Plate**. Mix thoroughly by pipetting up and down ten times at 4 μ l, being careful not to introduce excessive bubbles. Use clean tips for addition of each DNA sample.

Optional: If excessive bubbles are present after reaction set-up, use a tabletop centrifuge to collapse the bubbles prior to proceeding.

- e. After mixing all the reaction components and DNA together in the **Reaction Ready Plate**, transfer all the contents (16 μ l) to a clean 8-tube PCR strip(s) or a clean PCR plate.
- f. Seal tubes or the plate and spin down briefly.
- g. After verifying that the seals on the unused portion of the **Indexing Reagent Plate** and **Ready Reaction Plate** are still intact, cover the used wells to prevent contamination of the unused reagents when the plates are handled again. Then return the sealed/resealed plates to the freezer for later use.
- h. Proceed directly to [Section 2: Thermal Cycling on Page 18](#).

1C. ExpressPlex Reaction Setup (Using Automated liquid handlers)

ExpressPlex reactions can be set up at room temperature directly in the **Ready Reaction Plate** using a 96-channel pipetting head, an 8-channel pipetting head, or even an automated single-channel pipetting device. By using the same pipette tips to aspirate indexing reagents and the DNA samples, also known as the *EP Green Method*, the plastic consumables and time required for setup can be dramatically reduced (see the [EP Green Automation Workflow Diagram](#)). Optimal throughput is achieved using 96-channel instruments.

- a. Pre-label each **Ready Reaction Plate** with the number from the **Indexing Reagent Plate** and a name to allow easy identification of your samples.
- b. Pulse-spin one **Indexing Reagent Plate** and one **Ready Reaction Plate** in a tabletop centrifuge and remove the heat seals carefully.
- c. Aspirate 4 μ l of approximately 1.25 ng/ μ l input DNA into all channels of the pipettor. Using the same tips, aspirate 4 μ l of **Indexing Reagent** into all channels of the pipettor.

NOTE: *Sufficient overage is provided to reliably aspirate 4 μ l of **Indexing Reagent**, however each well of the **Indexing Reagent Plate** is intended for one use only.*

- d. Dispense 8 μ l from the tips into the **Ready Reaction Plate**.
- e. Mix thoroughly by rapidly aspirating and dispensing an 8 μ l volume ten times, being careful not to introduce bubbles. If excessive bubbles are present after reaction setup, use a tabletop centrifuge to collapse the bubbles prior to proceeding.
- f. Seal the **Ready Reaction Plate**, transfer to a thermal cycler, and proceed directly to [Section 2: Thermal Cycling on Page 18](#).

2. Thermal Cycling

- a. Transfer the plate or strip-tube(s) containing the assembled reactions to a thermal cycler, and run the **EP2 TAG AMP** thermal cycling program below, with lid-heating set to 105°C:

15	min	55°C	Tagging Reaction
5	min	75°C	Heat Inactivation / Fill-in
3	min	68°C	
5	min	79°C	
3	min	68°C	
5	min	83°C	
1	min	98°C	Initial denaturation
15	sec	98°C	Library Amplification (PCR) Use 12 cycles for plasmids Use 15 cycles for amplicons
30	sec	64°C	
1	min	72°C	
5	min	72°C	Final extension
Hold		4°C	

SAFE STOPPING POINT

**Proceed immediately to the next step
or store the amplified libraries at -20°C.**

3. Library Pooling

- a. After library amplification, pulse-spin the **Ready Reaction Plate** and then remove the plate seal.
- b. Using a multichannel pipette or an automated 8-channel pipetting head, pool 10 μ l of each amplified library from each column into a single prelabeled 8-tube PCR strip. The same pipette tips may be used for pooling multiple reactions.

Optional: If processing multiple plates with a 96-channel pipetting head, stamp the contents of multiple 96-well plates into one 96-well PCR plate and mix by pipetting before pooling into four strip tubes and subsequently four 2 ml LoBind tubes.

- c. After mixing by pipetting, transfer the entire volume from each well of the 8-tube PCR strip(s) into a prelabeled 2 ml LoBind tube.

If excessive bubbles are present after pooling, use a tabletop centrifuge to collapse the bubbles prior to proceeding. User may freeze any unpurified amplified libraries remaining in the **Ready Reaction Plate**, providing an option to purify more libraries later if any sample(s) should require additional sequencing depth.

4. Library Pool Purification

- a. Ensure MAGwise beads have been equilibrated to room temperature for at least 30 minutes before use.
- b. Vortex the room temperature MAGwise to ensure that the beads are fully resuspended before use.
- c. To the pooled ExpressPlex libraries made in the previous section, add 0.75X volumetric equivalent of **MAGwise** (e.g., add 720 µl of MAGwise to 960 µl of pooled library). To determine this volume, measure the volume of the pooled library via reverse pipetting, and multiply that volume by 0.75.

For libraries derived from amplicons, use 1 volumetric equivalent of **MAGwise** in order to recover the shorter fragments.

- d. Add MAGwise and mix thoroughly by pipetting up and down $\geq 10\times$. Incubate on the bench for 5 minutes to allow the DNA to bind.
- e. Place the tube on a magnetic stand and let the bead pellet form on one side of the tube and wait until the supernatant appears completely clear (5 minutes or less).
- f. Remove and discard the supernatant with pipette. Be careful not to disturb the bead pellet.
- g. Wash beads with 80% ethanol.
 - i. With the tube in the magnetic stand, add sufficient 80% ethanol to cover the bead pellet, without disturbing the bead pellet.
 - ii. After ≥ 30 seconds, remove and discard the supernatant, without disturbing the bead pellet.
- h. Repeat the previous step for a total of 2 washes with 80% ethanol. [**Do not air dry the bead pellets---proceed immediately to the next step**]

Useful tip: After using a large pipette tip to remove the waste ethanol from the second wash, briefly pulse-spin, return to the magnet, and then use a smaller pipette tip to remove any residual volume, if visible.

- i. Immediately remove the tube from magnetic stand and pipette 30 µl of 10 mM Tris-

HCl, pH 8 on top of the bead pellet. Pipette the solution along the inner wall of the tube multiple times to thoroughly resuspend the bead pellet.

Optional: Lower elution volumes (<30 µl) can be used to increase the concentration of libraries prepared from fewer than 48 samples. Fewer than 16 samples may be processed ONLY IF an experienced user is comfortable with a final elution volume of 15 µl.

- j. Incubate the tube on the bench for at least 5 minutes to elute the libraries from the beads.
- k. Return tube to magnetic stand and allow the bead pellet to reform on the inner wall of the tube (~2 minutes).
- l. When the supernatant has cleared completely, carefully transfer the DNA eluate to a clean 1.5 ml LoBind tube. The transferred eluate contains the purified pooled library.

SAFE STOPPING POINT

**Proceed immediately to the next step
or store the pooled purified library at -20°C.**

Library Quantification and QC

Library quantification and QC with electrophoretic analysis: Run the pooled, purified ExpressPlex 2.0 library on the Agilent TapeStation (High Sensitivity D5000 kit), Bioanalyzer (High Sensitivity DNA or DNA7500 kits), or Fragment Analyzer (High Sensitivity NGS Fragment Analysis Kit, DNF-474) following the manufacturer's instructions for these instruments. For optimal sequencing results with ExpressPlex 2.0 plasmid libraries, use a region analysis for fragments of **200 - 1,200 bp** to determine the average clusterable fragment length for size adjustment. For amplicon libraries, adjust the region size based on the input amplicon length to exclude unfragmented amplicons.

If using electrophoretic analysis for library quantification, use the region analysis function and calculate the library concentration from the clusterable fragment region. Alternatively, use Quant-iT PicoGreen dsDNA Assay, Qubit dsDNA HS Assay (see below) or other validated dsDNA quantification assay to quantify the library pool, and calculate amount of clusterable fragments by multiplying by the percentage of sample in the region analysis (200-1200bp) for sequencer loading. For a more accurate measurement of the concentration of clusterable library fragments, use qPCR (see below).

Refer to the figures below for representative trace for pooled, purified libraries run on the TapeStation. Refer to [Appendix D](#) for quantification methods by Agilent TapeStation for ExpressPlex 2.0 libraries.

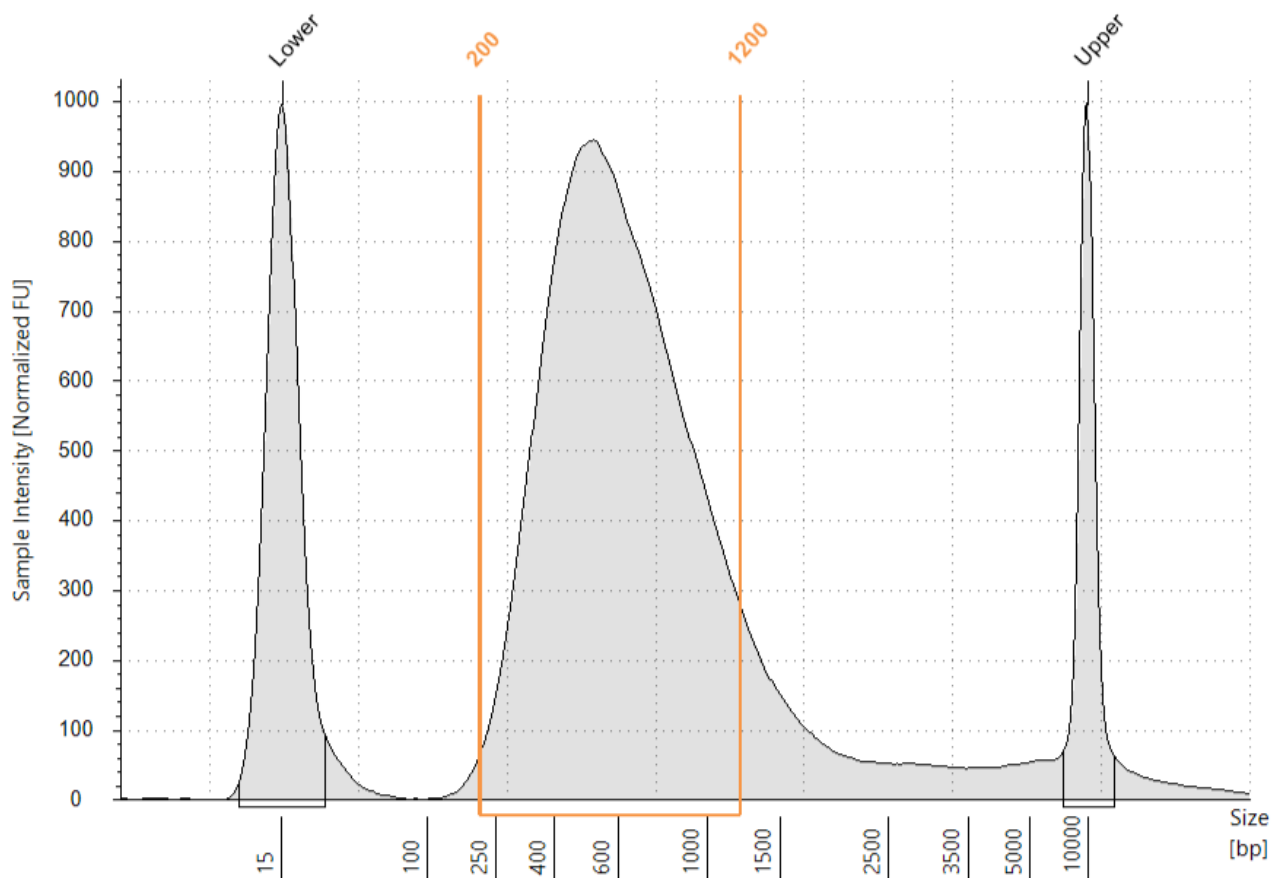


Figure 1. Representative TapeStation electropherogram of a pooled, purified ExpressPlex 2.0 plasmid library (diluted 20-fold prior to electrophoresis). The analysis region (orange) shows the range of clusterable fragments.

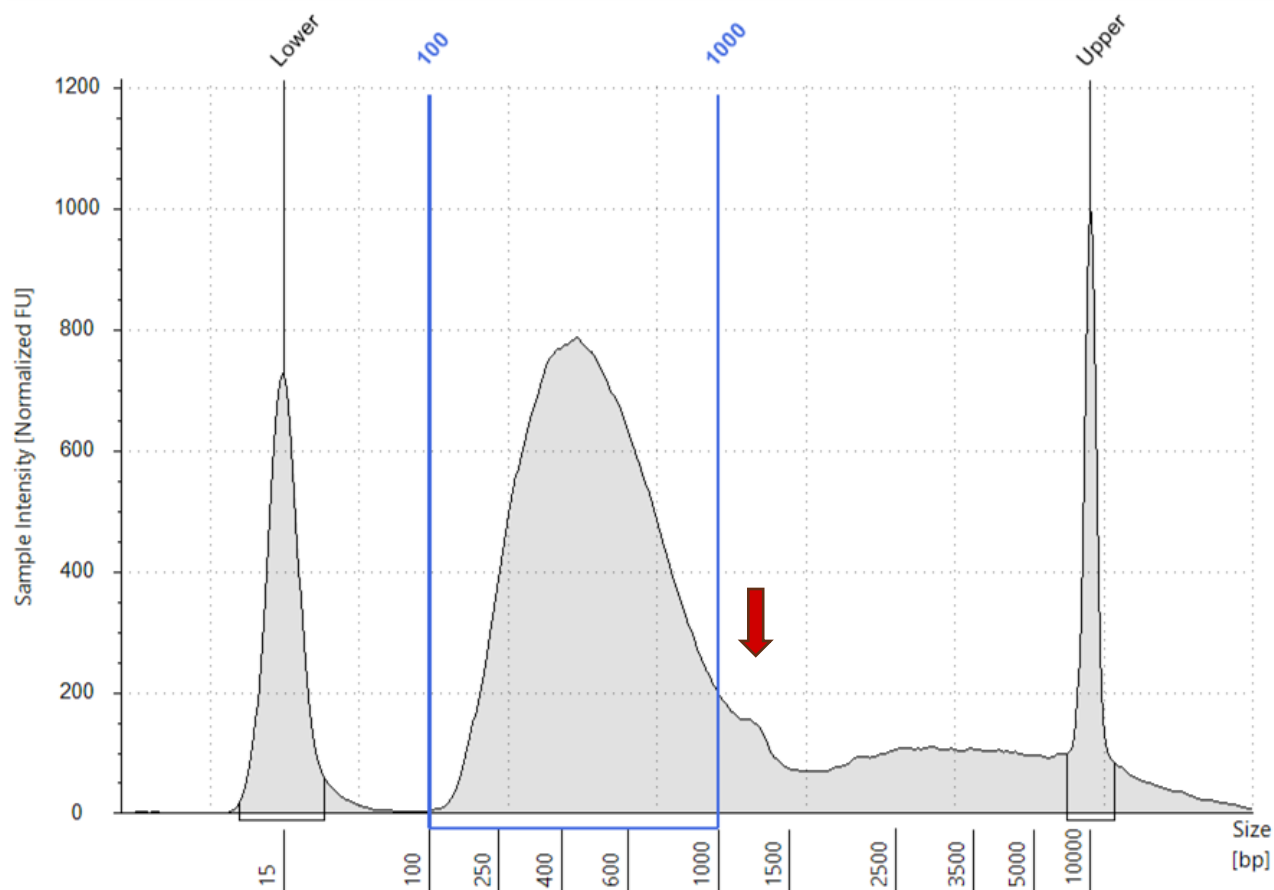


Figure 2. Representative TapeStation electropherogram of a pooled, purified ExpressPlex 2.0 amplicon library (diluted 20-fold prior to electrophoresis). The analysis region (blue) shows the range of clusterable fragments. Arrow (red) shows a small amount of unfragmented amplicon DNA.

Library quantification with dsDNA specific fluorometric method: ExpressPlex 2.0 libraries are double stranded. Use 2 µL to quantify the pooled, purified library using the Qubit dsDNA assay, Quant-iT PicoGreen dsDNA assay or other validated dsDNA quantification assay. Follow the manufacturers' instructions for the appropriate dilutions. Use the average clusterable fragment size as determined by electrophoresis to calculate the library concentration and the dilution factor required for loading your sequencing system.

Library quantification with qPCR assay: qPCR is a very sensitive method of quantifying library fragments that have both adaptor sequences on either end which will subsequently form clusters on a flow cell. Use 2 µl of the purified, multiplexed ExpressPlex 2.0 library for qPCR analysis with Illumina qPCR primer 1.1/2.1 1 described on Illumina's website here:

(https://support.illumina.com/content/dam/illumina-support/documents/documentation/chemistry_documentation/qpcr/sequencing-library-qpcr-quantification-guide-11322363-c.pdf). Follow kit and instrument instructions for appropriate conditions and dilutions.

Sequencing on Illumina platforms

Read configuration: ExpressPlex Library Prep kit libraries are dual indexed with 10 base indexes. Index lists can be found in [Appendix C](#) and in the index spreadsheet on the [seqWell website](#). ExpressPlex libraries are sequenced using the same primers as standard Illumina libraries, and consequently, custom sequencing primers are not needed. Longer reads deliver greater read depth, and read lengths of 2 x 150 or greater are recommended for *de novo* assembly. The i7 and i5 index reads must be 10 bases long for ExpressPlex libraries, although the index reads and non-index reads can be adjusted for different sequencing kits, speed, or read depth requirements. For example, the sequencing run can be demultiplexed using only the unique i7 barcodes when running 96 or fewer ExpressPlex libraries with a single i5 on a sequencer.

Library dilution, denature and sequencing: Follow Illumina's guidelines for appropriate dilution to the starting concentration and loading procedures specific to your sequencing system. Not all DNA fragments can efficiently generate clusters. Longer library fragments generally do not cluster as efficiently on a flow cell. It is essential to optimize the loading concentration based on your sample type, library QC methods, and library fragment distribution. Try adjusting loading concentration over subsequent sequencing runs to optimize cluster density and sequencing run performance.

Add PhiRx Indexed Control to library pool. See [Appendix E](#) for instructions.

Appendix A: Adjusting the Input Sample Concentration

ExpressPlex 2.0 (96-well) Library Preparation Kits perform optimally with 1 - 40 ng of total dsDNA input per 16 μ l reaction, and individual adjustment of each sample concentration is not necessary.

If the method used to purify DNA upstream of library prep is well-characterized and generates relatively consistent concentrations of DNA per sample, it may be sufficient to only assay several samples from the DNA sample plate (*i.e.*, spot-check the dsDNA concentration using a PicoGreen Assay to estimate the average DNA concentration across all samples).

If all of the samples already fall within the 0.25 – 10 ng/ μ l range, no adjustment is required. If, however, the average concentration of all of the samples exceeds 5 ng/ μ l, calculate the global dilution factor using the formula below:

$$\text{Global dilution factor (X)} = \frac{\text{Average assayed dsDNA concentration (ng/\mu l)}}{1.25 \text{ ng/\mu l}}$$

The global dilution factor is applied to the input samples so that the average DNA concentration across all samples will be approximately 1.25 ng/ μ l (*i.e.*, resulting in an average of 5 ng of input being added per full ExpressPlex reaction volume).

NOTE: *If the DNA concentration of the input samples is not easily confined to an approximately 40-fold range (maximum concentration divided by minimum concentration), or, if an average sample concentration of ≥ 0.25 ng/ μ l cannot be routinely achieved, consider optimizing the method used to generate input DNA.*

Important Reminder: Do not use EDTA-containing solutions (*e.g.*, TE buffer) to dissolve or dilute input DNA because EDTA can suppress enzymatic activity.

Appendix B: Sample Sheet and Sequencer Guidelines

Illumina sequencing systems and chemistries differ in their use of sample sheets, availability of on-instrument demultiplexing, optimal color balancing, and run setup methods. If you have questions for your specific sequencer, contact Illumina technical support for the best guidance on setting up your run using your sequencing platform.

ExpressPlex 2.0 libraries are similar to the Nextera Adapter sequences and are dual-indexed using 10 base indexes for both the i7 and i5 index sequences. ExpressPlex libraries do NOT require custom sequencing primers.

All Illumina sequencers read the i7 index in the forward direction (as listed in [Appendix C](#)). The i5 index, however, is read differently on different sequencers depending on the version/chemistry of the sequencing kits. In this case, if using an Illumina sample sheet template, enter the i5 index in the forward direction as the sample sheet will auto-generate the reverse complement if needed. If demultiplexing using bcl2fastq and using a sequencer that reads the reverse complement of the i5 index sequence, enter the reverse complement of the i5 index shown in the ExpressPlex 2.0 index list on seqWell's website: <https://seqwell.com/expressplex-2-0-library-prep-kit/>.

Please refer to Illumina's website for most up to do index sequencing guidelines:

<https://support.illumina.com/downloads/indexed-sequencing-overview-15057455.html>

Appendix C: ExpressPlex Index Information and Demultiplexing Guidance

ExpressPlex utilizes a combinatorial dual indexing (CDI) strategy: all 16 Indexing Reagent Plates have the same 96 i7 indexes but each plate has a different i5 index, providing 1,536 barcode combinations in total. For a complete list of all i7 indexes (listed by row and column formats as well as in plate layout) and the i5 indexes, please refer to the ExpressPlex 2.0 index list in spreadsheet format on seqWell's website: <https://seqwell.com/expressplex-2-0-library-prep-kit/>.

i7 Index Plate Map for ExpressPlex

	1	2	3	4	5	6	7	8	9	10	11	12
A	GTCAAGTCCA	CAACTAATC	ATAACCTGAC	CAGGTACTTC	AACCGAGCCA	CAACGTCATT	ATTGGTCAGA	ATGTTGCGGA	CACCAATAAC	TGTCGGTCTT	CGAAGGACTG	TAGTTATCGC
B	TATCTCTTCC	GTAAGTGGAT	TGCGGTTCCA	CAGGAATATG	TGGATTCAAG	AAGAACGATG	AAGACCTGTT	AATGCTAACC	GCGTCCACAA	CATGAGTAAC	TCTACCGTCA	TGCAGGTGAT
C	CGCGAAGAA	CATCGGAGGA	AATACTTGCC	AACGCACAAT	CAACAGATAC	CTGCAATTAC	CGCTAATGAA	GTAACACGTA	ATGTGCGCTT	CTGCGCGAAT	GGTAATATCG	TGTGAAGCTA
D	CCTACTCGGA	ATTCTGATGG	AATCGCGGAA	ATTGAGAAGG	AAGGTAACCTC	CGCCGATGAT	CAGAGTGTCAT	GATATACGGA	TATCTAGTGC	CTGTAGTATG	TGTGCGAGTT	CAACTCCTGA
E	TTGCTATCAC	TATCGTTACC	CAGAACGCGA	ATTGCACCTT	TGACAATACG	CGGACAAGAC	GGTAAGCTGA	ATCCGAGAGG	GCCTACAATG	GAGCCGTACA	TTATCGCTGA	TGTAGCAACG
F	TCCTCCATCC	TGGTCTGTTA	TGAACCAAGG	AAGTGGATAC	GATTGTGCAT	CGTACTCCTC	GTATTCACTG	CAATTACACAC	AAGCTCAGTT	CATTCTTAGG	GGTTGAGTTC	CGGTAACGCA
G	ATAACATCGC	TGCCAACATG	TGTTAGTCAG	GATAAGATGC	GCACACCATT	TGCATGAGTT	GCGCTACGTT	TTGTCAGTTC	TACGCTTAGA	TGACCGACAA	ATTGGACGCC	GTAGCAGCAG
H	GATATGCGTT	TCATTACAG	CAGTAGGTAA	TACCTCGACA	TCGTTATTCC	AATCTGGAGC	TTGTCATAGC	ATACGCCATT	ATCCACTAGG	TGTGTAACCG	TATGTGTGTG	CTACAGCCGA

i5 Index Read

Set	Index name	i5 forward*	i5 reverse*
Set A	1001	GTAAACAGAG	TCTGTGTTAC
	1002	CAAGAGCGTG	CACGCTCTTG
	1003	CCGAGGTTAG	CTAACCTCGG
	1004	TGGAGCGATG	CATCGCTCCA
Set B	2001	ATCTCCACGG	CCGTGGAGAT
	2002	ATTCCGCTTA	TAAGCGGAAT
	2003	TTGTTCTGCG	CGCAGAACAA
	2004	CCTCTGAACA	TGTTCAAGAG
Set C	3001	CTGATTAGGA	TCCTAATCAG
	3002	CAATGCGGAG	CTCCGCATTG
	3003	GTATCTTAGG	CCTAAGATAC
	3004	TCGCGGACAT	ATGTCCCGCA
Set D	4001	TAAGTTGTGG	CCACAACCTA
	4002	CCGTAATCGA	TCGATTACGG
	4003	CTCAGTAGAC	GTCTACTGAG
	4004	CTTATCCAGG	CCTGGATAAG

Important Note: Illumina sample sheets for on-board demultiplexing use the i5 index forward read sequence. The software will automatically generate the reverse complement for sequencers that rely on the i5 index reverse read sequence. Please refer to Illumina's recommendations for optimal color balancing for different sequencing chemistries.

Optimal Demultiplexing Guidance:

In accordance with Illumina's guidelines, it is recommended to allow for 1 mismatch in the barcode reads during demultiplexing. This allows for the capture of many more reads than 0 mismatch at a reduced risk, due to sufficient Hamming distances between barcodes.

Refer to *Illumina's mismatch guidelines here*:

https://knowledge.illumina.com/software/general/software-general-reference_material-list/000007484

For the XLEAP chemistries:

For NovaSeq X, NextSeq 2000, and MiSeq i100 running XLEAP-SBS chemistry, an increased rate of 1 mismatch in the barcode reads has been observed. Hence, it is especially important to allow for 1 mismatch on these instruments to recover all expected data for each barcode.

Appendix D: Library Quantification Options

In this example, Agilent TapeStation was employed to quantify a pooled, purified plasmid ExpressPlex 2.0 library for sequencer loading.

Refer to the figure below for library QC results.

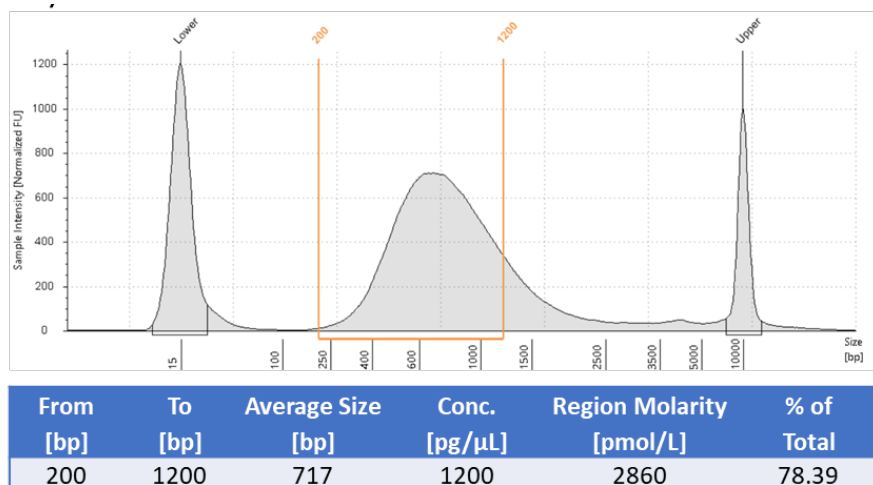


Figure 3. Example of library quantification results for a pooled, purified plasmid library by Library QC on Agilent TapeStation.

Use the following formula to convert library concentration from ng/μl to nM:

$$\text{Library concentration [nM]} = \frac{\text{Library concentration} \left[\frac{\text{ng}}{\mu\text{L}} \right]}{660 \left[\frac{\text{g}}{\text{mol}} \right] \times \text{Average fragment size [bp]}} \times 10^6$$

Library quantification by TapeStation **ONLY** (Library diluted 20-fold prior to electrophoresis):

- Clusterable region average library size: 717 bp
- Clusterable region library concentration: 1200 pg/μl × 20 = 24.0 ng/μl
- Estimated library concentration: $\frac{24.0 \left[\frac{\text{ng}}{\mu\text{L}} \right]}{660 \left[\frac{\text{g}}{\text{mol}} \right] \times 717 \text{ [bp]}} \times 10^6 = 50.7 \text{ nM}$

Appendix E: Using PhiRx Indexed Control in Illumina sequencing

Each ExpressPlex 2.0 kit comes with a vial of PhiRx™ Indexed Control, which is a dual-indexed control library made from phiX174 genomic DNA and optimized for Illumina sequencing platforms, particularly two-color systems like XLEAP SBS chemistry on NextSeq 1000/2000, MiSeq i100 and NovaSeq X. By improving color balancing for combinatorial indexed ExpressPlex 2.0 libraries (where there are only 1-4 i5 indexes used), PhiRx Indexed Control ensures cleaner, more accurate sequencing results and can be used as a 1:1 substitution for Illumina's PhiX Control V3.

Before starting procedure:

Review FAQs. FAQs can be found here: <https://seqwell.com/resource-category/faqs/>.

Thaw and mix reagent. Thaw reagent if necessary, pulse-spin down, and keep on ice. Pipette mix 10x before using.

Procedure

1. Dilution, aliquoting and denaturation

Please refer to Illumina's sequencer-specific recommendations for dilution and loading: <https://knowledge.illumina.com/instrumentation/general>.

PhiRx Indexed Control is a **non-denatured**, double-stranded library that is ready to be mixed with **non-denatured** target libraries. For applications requiring a denatured format, PhiRx Indexed Control can also be denatured following standard procedures and mixed exclusively with other **denatured** libraries.

Follow the procedure below for proper dilution, aliquoting, and storage:

a. Non-Denatured Use

- i. **Determine Concentration:** Select the appropriate concentration and aliquot volume based on your sequencing run's loading requirements.
- ii. **Low-Concentration Dilutions:** For dilutions below 1 nM, prepare aliquots sized for 1–2 weeks of use. Store long-term aliquots at -20°C, keeping only the aliquot in active use at 4°C.

b. Denatured Use

- i. **Dilution and Denaturation:** Dilute PhiRx Indexed Control to the required concentration, then denature according to Illumina's standard protocol, mixing by vortex and briefly spinning down.
- ii. **Storage:** Store the denatured PhiRx Indexed Control at -20°C. Prepare single-use aliquots, discarding any leftover volume after loading to prevent freeze-thaw degradation.

2. Sequencing on Illumina platforms

Check Illumina recommendations specific to your sequencing platform and analysis software version to determine the appropriate PhiRx Indexed Control spike-in percentage.

Recommended Spike-In Ratios by Application:

- a. **For Sequencing Quality Monitoring:** Add 1–2% of PhiRx Indexed Control to the target library.
- b. **For Color Balancing of Index Reads with XLEAP-SBS:** Begin with 5–10% PhiRx Indexed Control. Per Illumina's recommendation for their PhiX Sequencing Control V3, using a higher percentage of PhiRx (up to 40%) may improve performance, especially with XLEAP-SBS 600-cycle kits.
- c. **For Low-Diversity Libraries (Color Balancing of Insert Reads):** Start with 15–20% PhiRx Indexed Control and adjust upward if needed to enhance sequencing performance.

3. Sample sheet setup and bioinformatics information

PhiRx Indexed Control is designed with randomized mixed bases at each index position, meaning it cannot be demultiplexed from the run as a distinct sample. As with PhiX Sequencing control V3, PhiRx reads will appear in the undetermined category after demultiplexing, so no additional information is required during sample sheet setup.

For additional support with read filtering or bioinformatics applications, please contact technical support at support@seqwell.com.

Technical Assistance

Please review FAQs at <https://seqwell.com/resource-category/faqs/>.

For additional technical assistance with ExpressPlex 2.0 Library Preparation, contact seqWell Technical Support.

E-mail: support@seqwell.com

Version	Release Date	Prior Version	Description of changes
v20251110	November 10, 2025	V20250103	• PhiRx Indexed Control component added to kit and instructions added in Appendix E. • Reorganized instructions for full/partial plates.
v20250103	January 3, 2025	N/A	First version

seqWell, Inc.

66 Cherry Hill Drive

Beverly, MA 01915

USA

+1-855-737-9355

<https://seqwell.com/>

© 2025 seqWell. All rights reserved.

For Research Use Only – Not for Diagnostic Use
UserGuide_EP9620251110

seqWell, the seqWell logo, TnX, PhiRx and ExpressPlex are trademarks of seqWell, Inc.
All other trademarks are property of their respective owners.